


Data : 2009/Reagents2:084
Sample : PS5200
Average(MS[1] Time:0.37..0.46)

Date : 2010/07/23 13:20:18

JEOL JMS-T100GCV : FD+
Detector Volt: 2100[V]

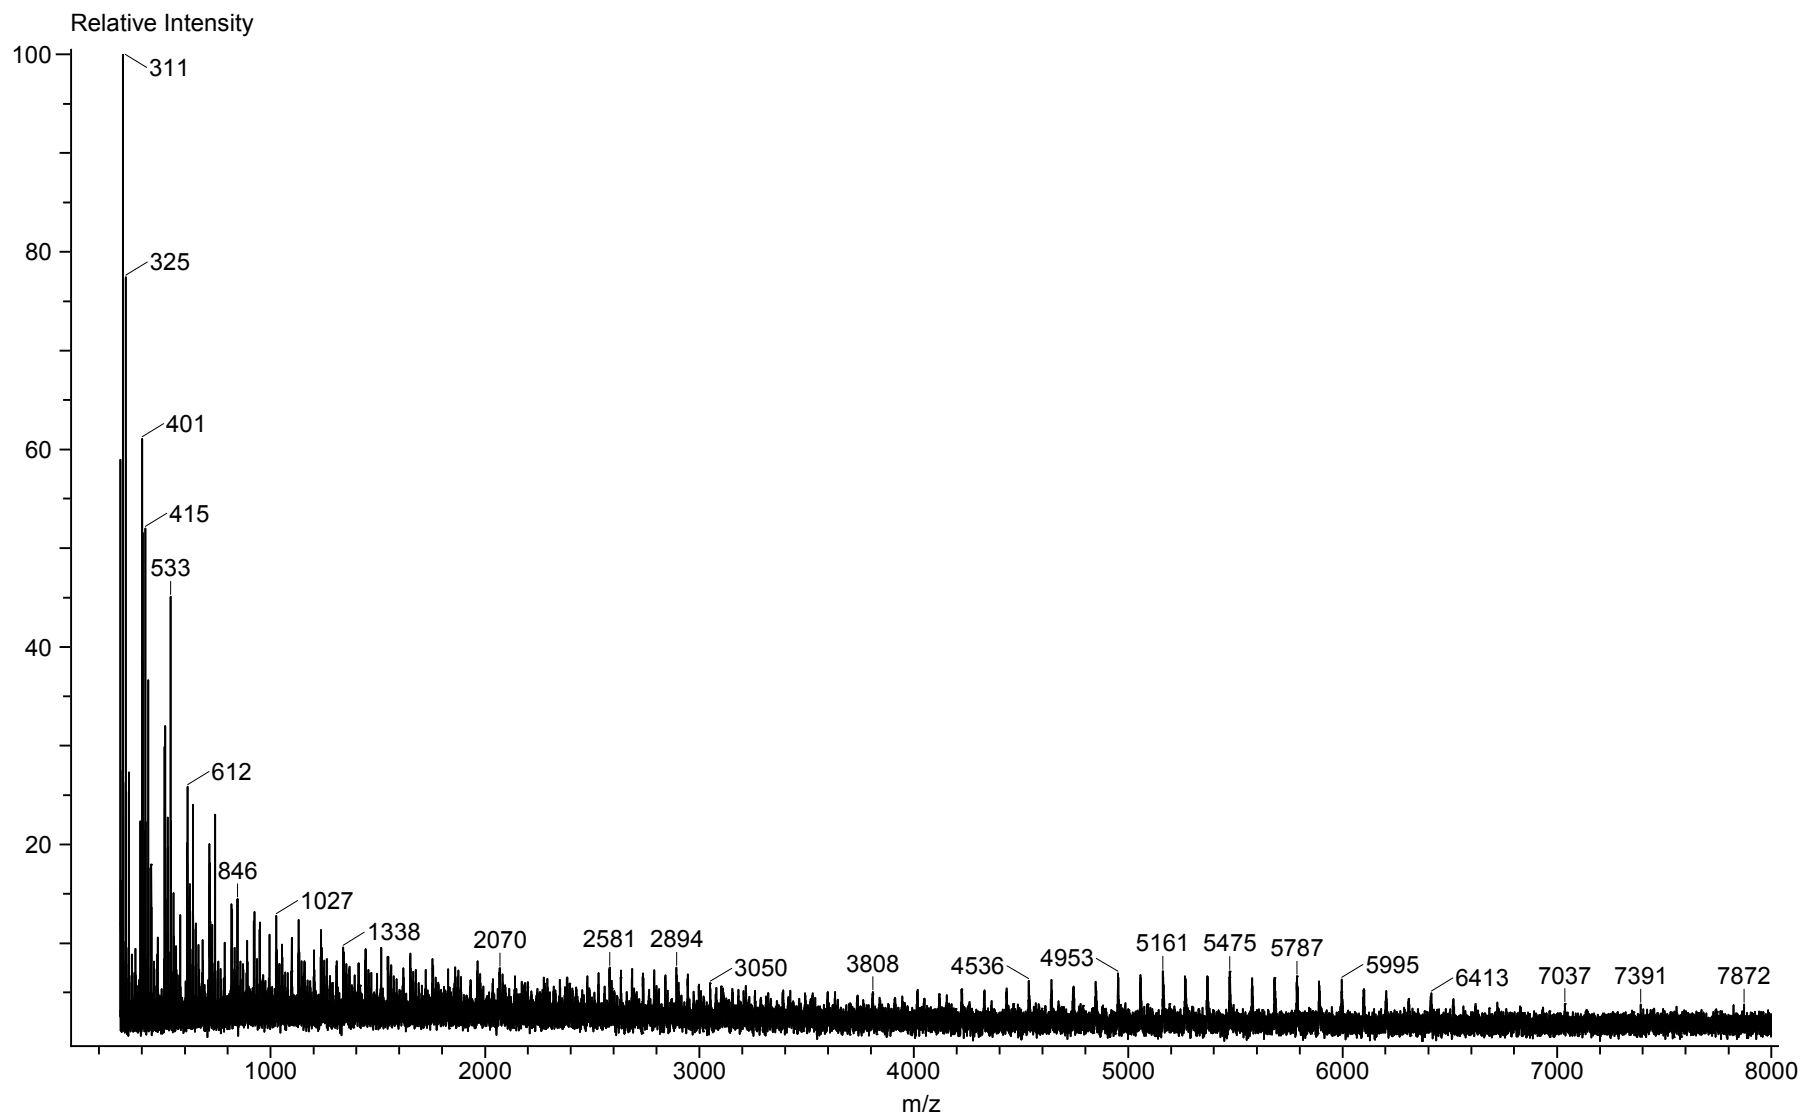

Data : 2009/Reagents2:084
Sample : PS5200
Average(MS[1] Time:0.37..0.46)

Date : 2010/07/23 13:20:18

JEOL JMS-T100GCV : FD+
Detector Volt: 2100[V]

